

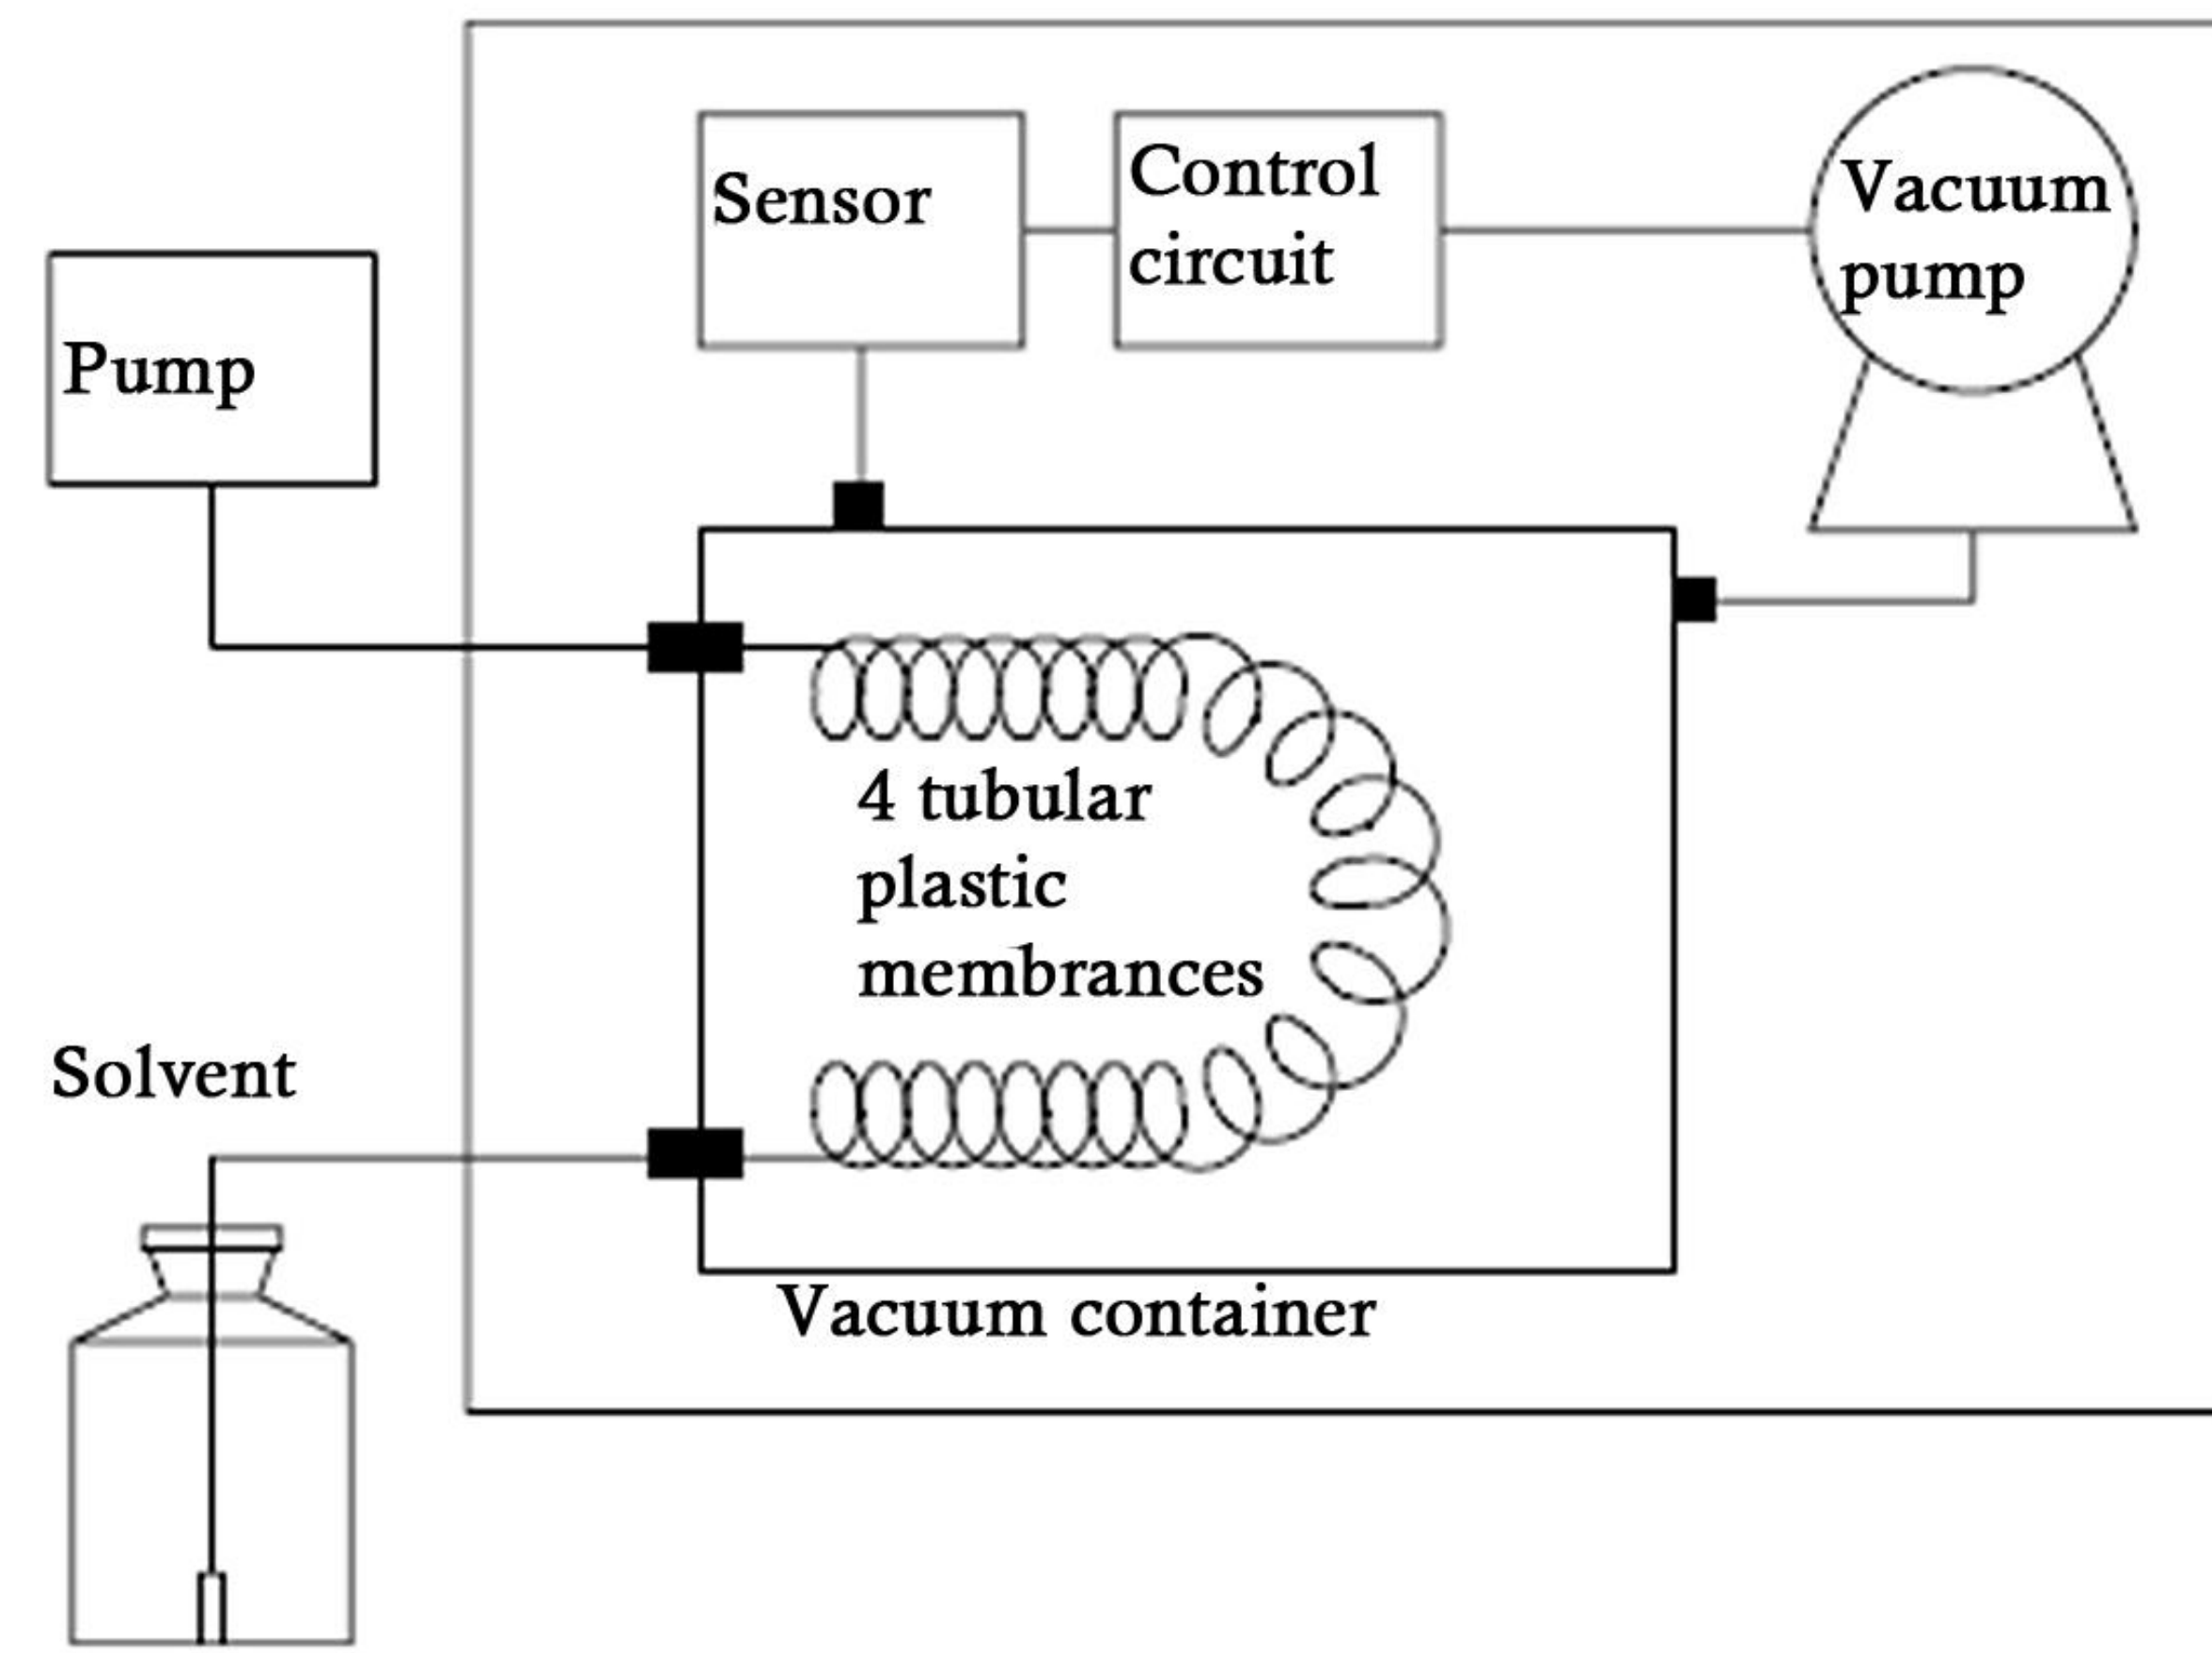



Agilent 1200 capillary LC components diagram

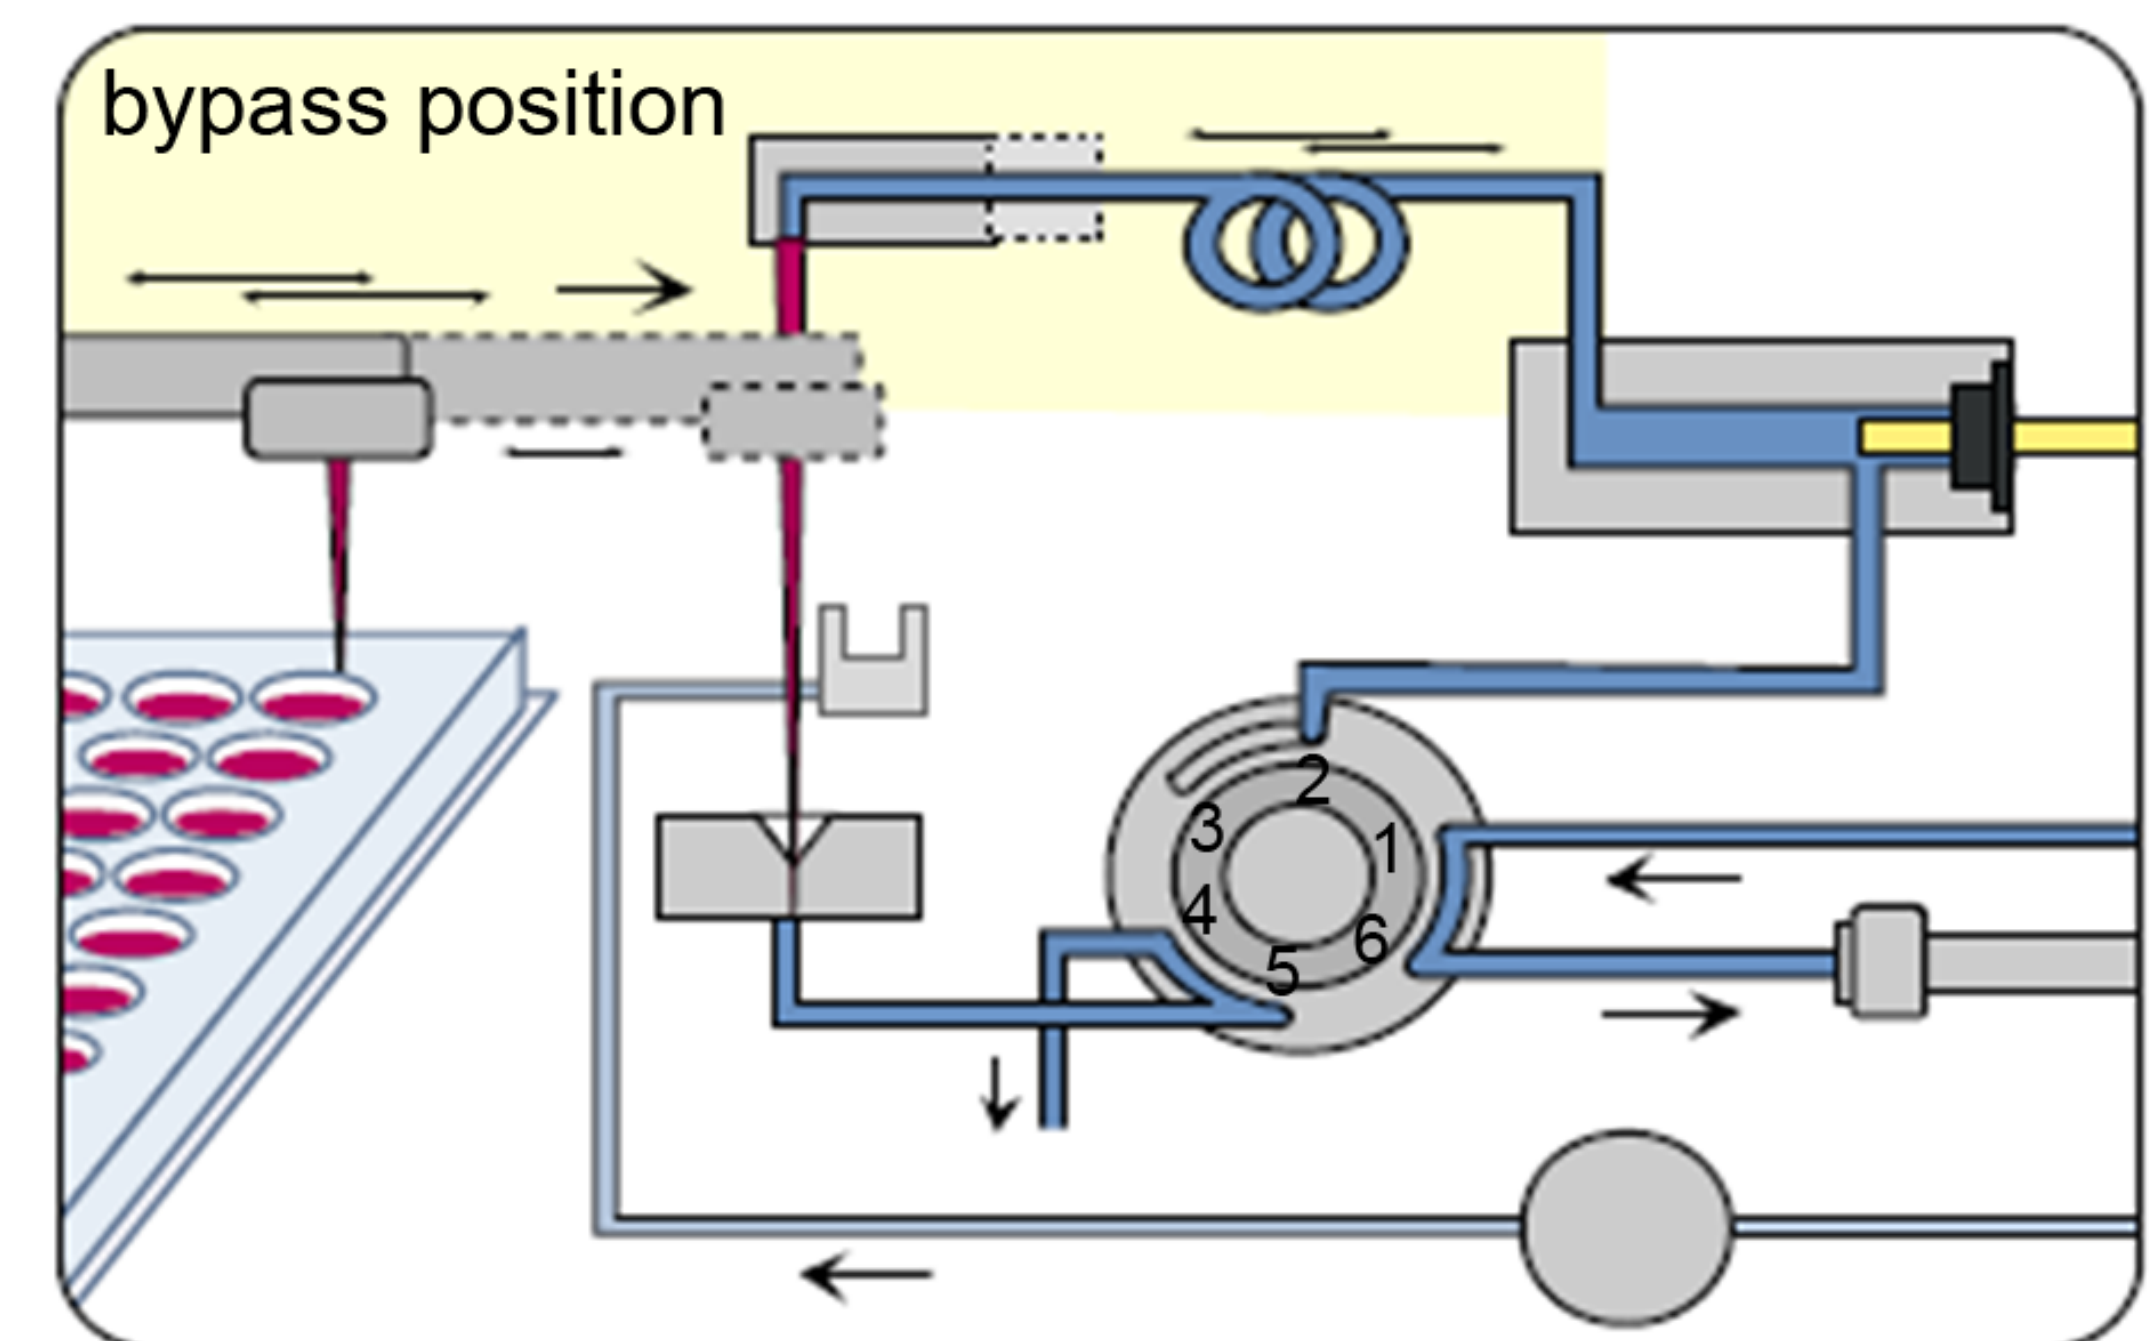

Vacuum degasser

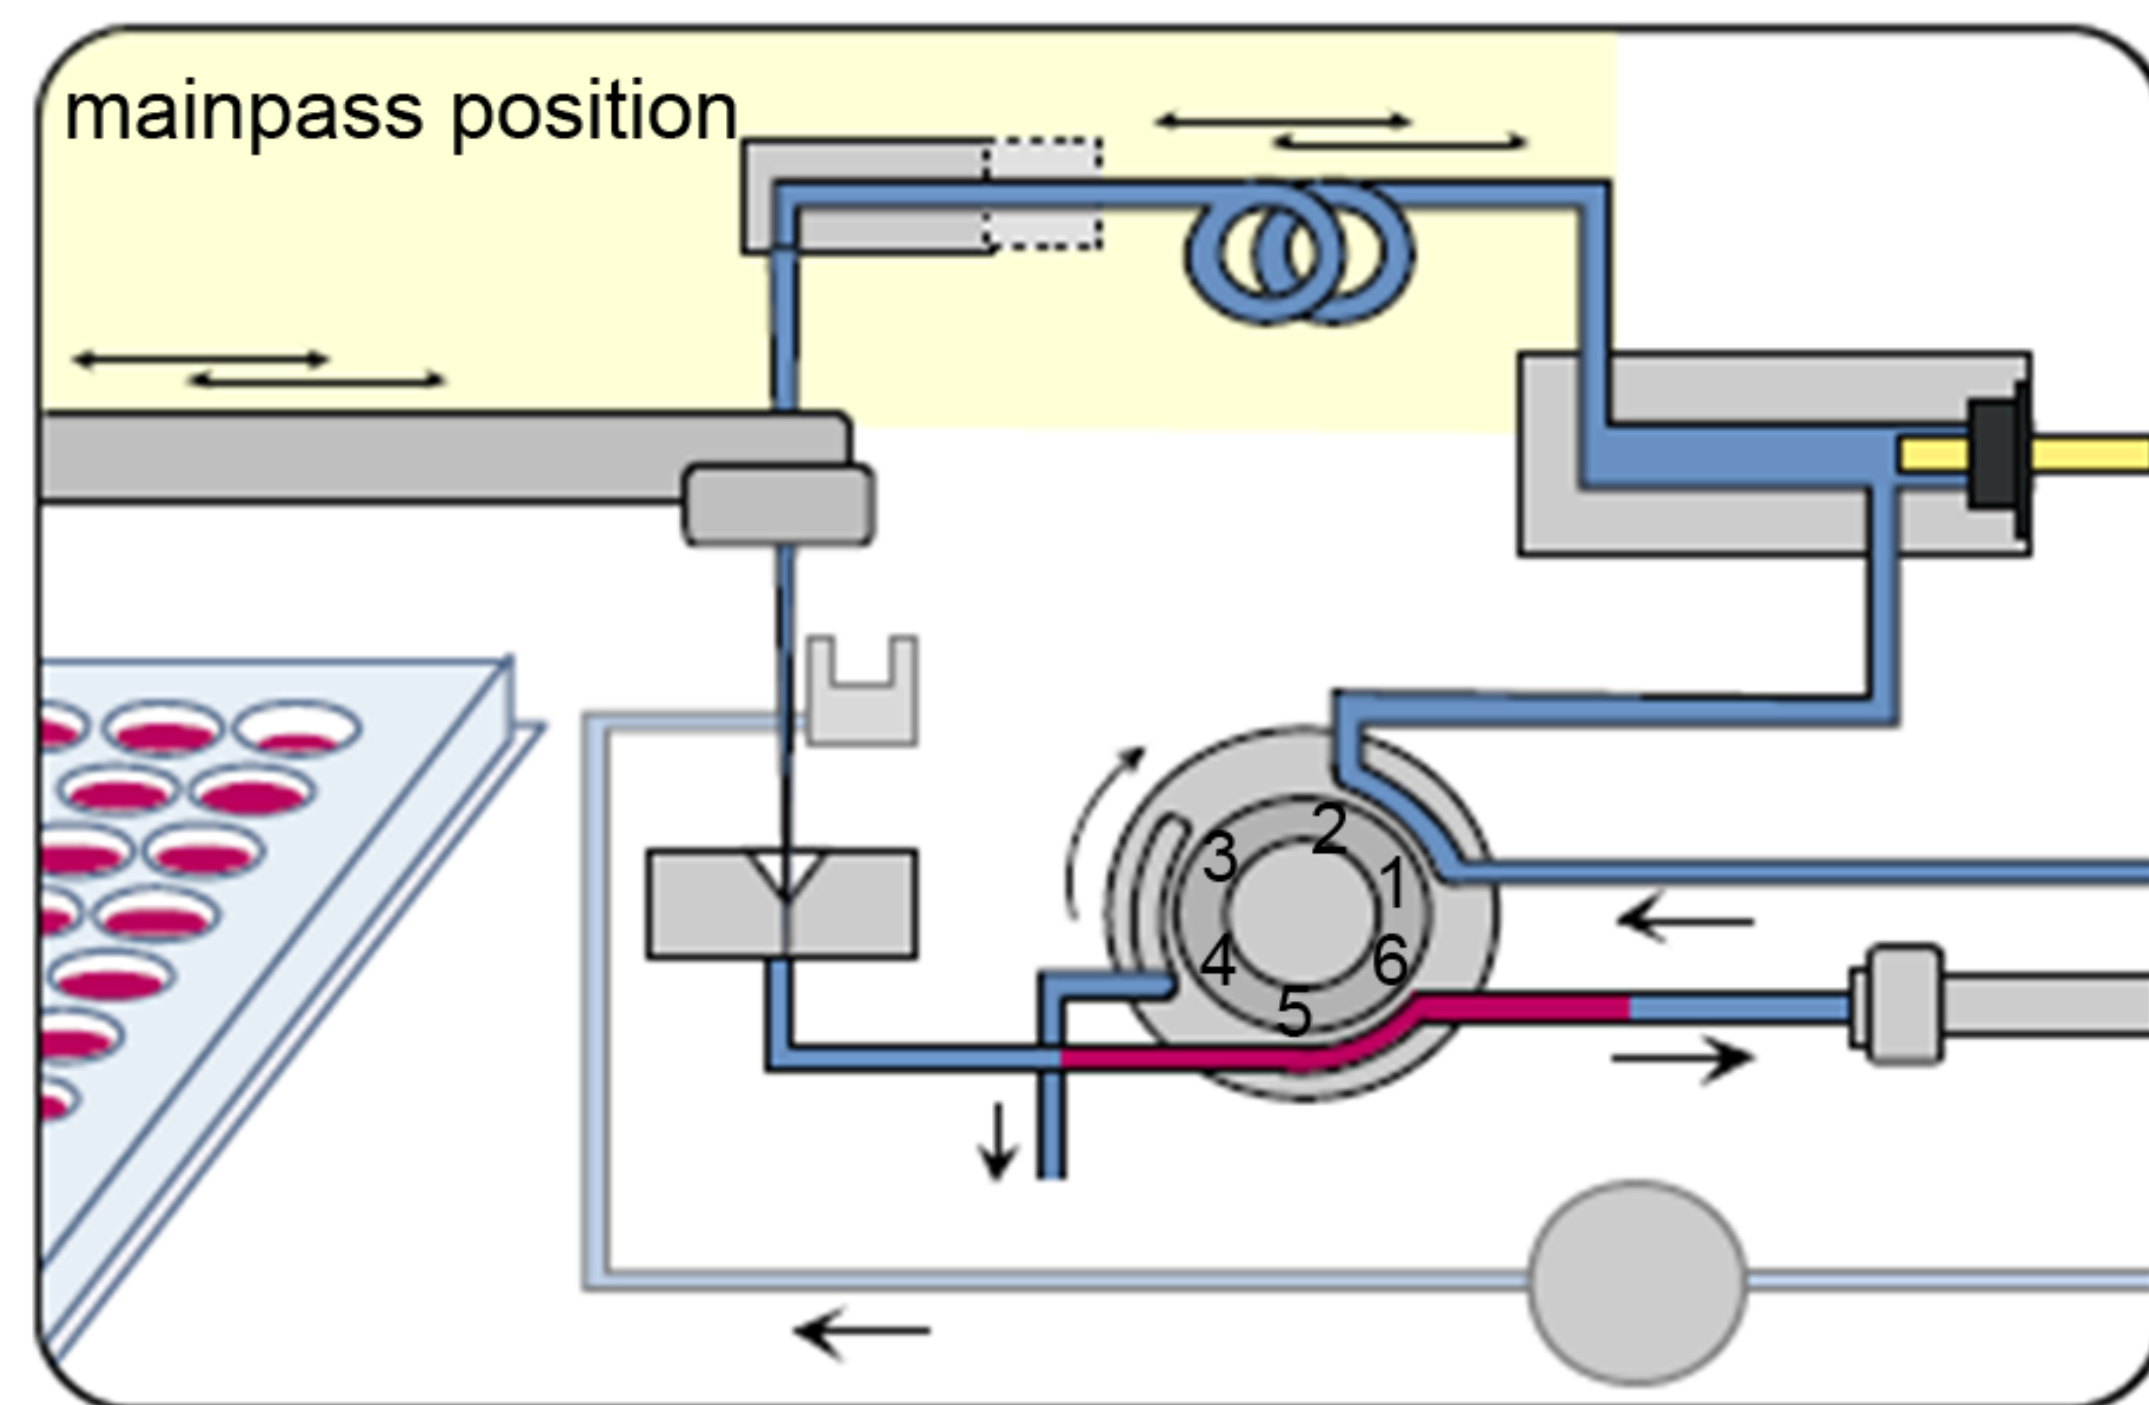


Autosampler injection sequence

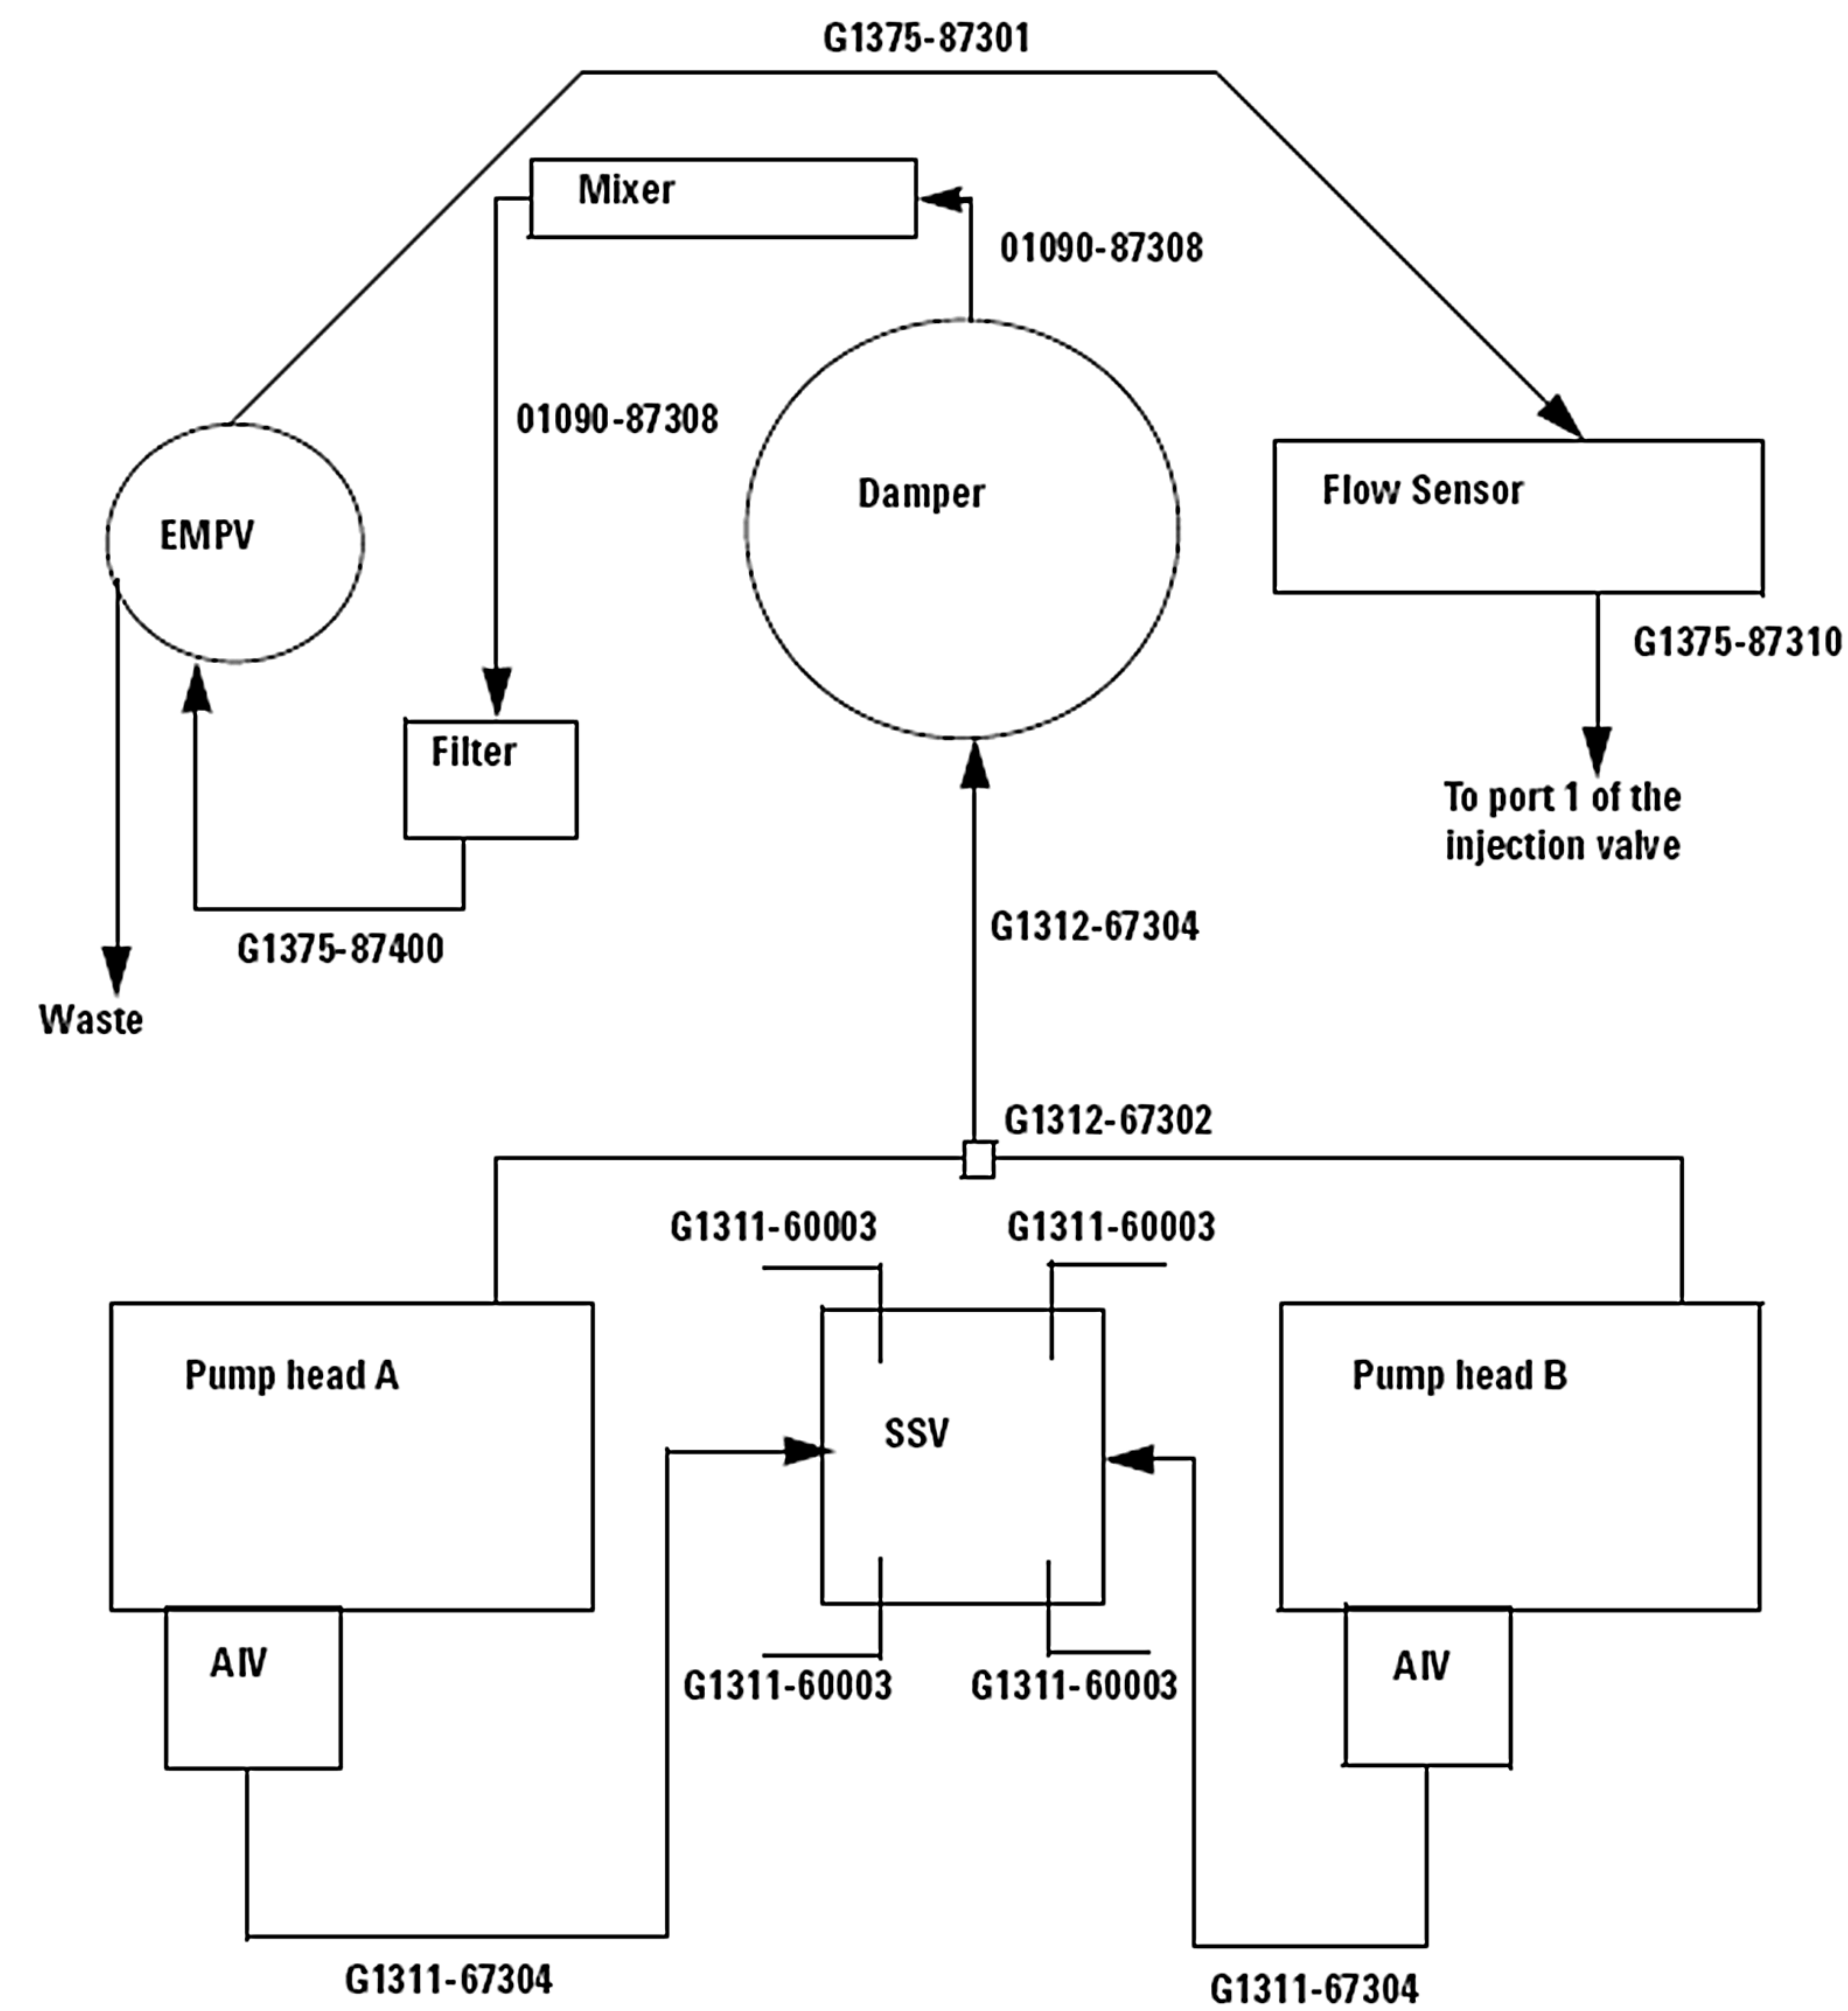

Pump flow connection

EMPV: Electro-Magnetic-Proportional-Valve
 SSV: Solvent-Selection-Valve
 AIV: Active-Inlet-Valve

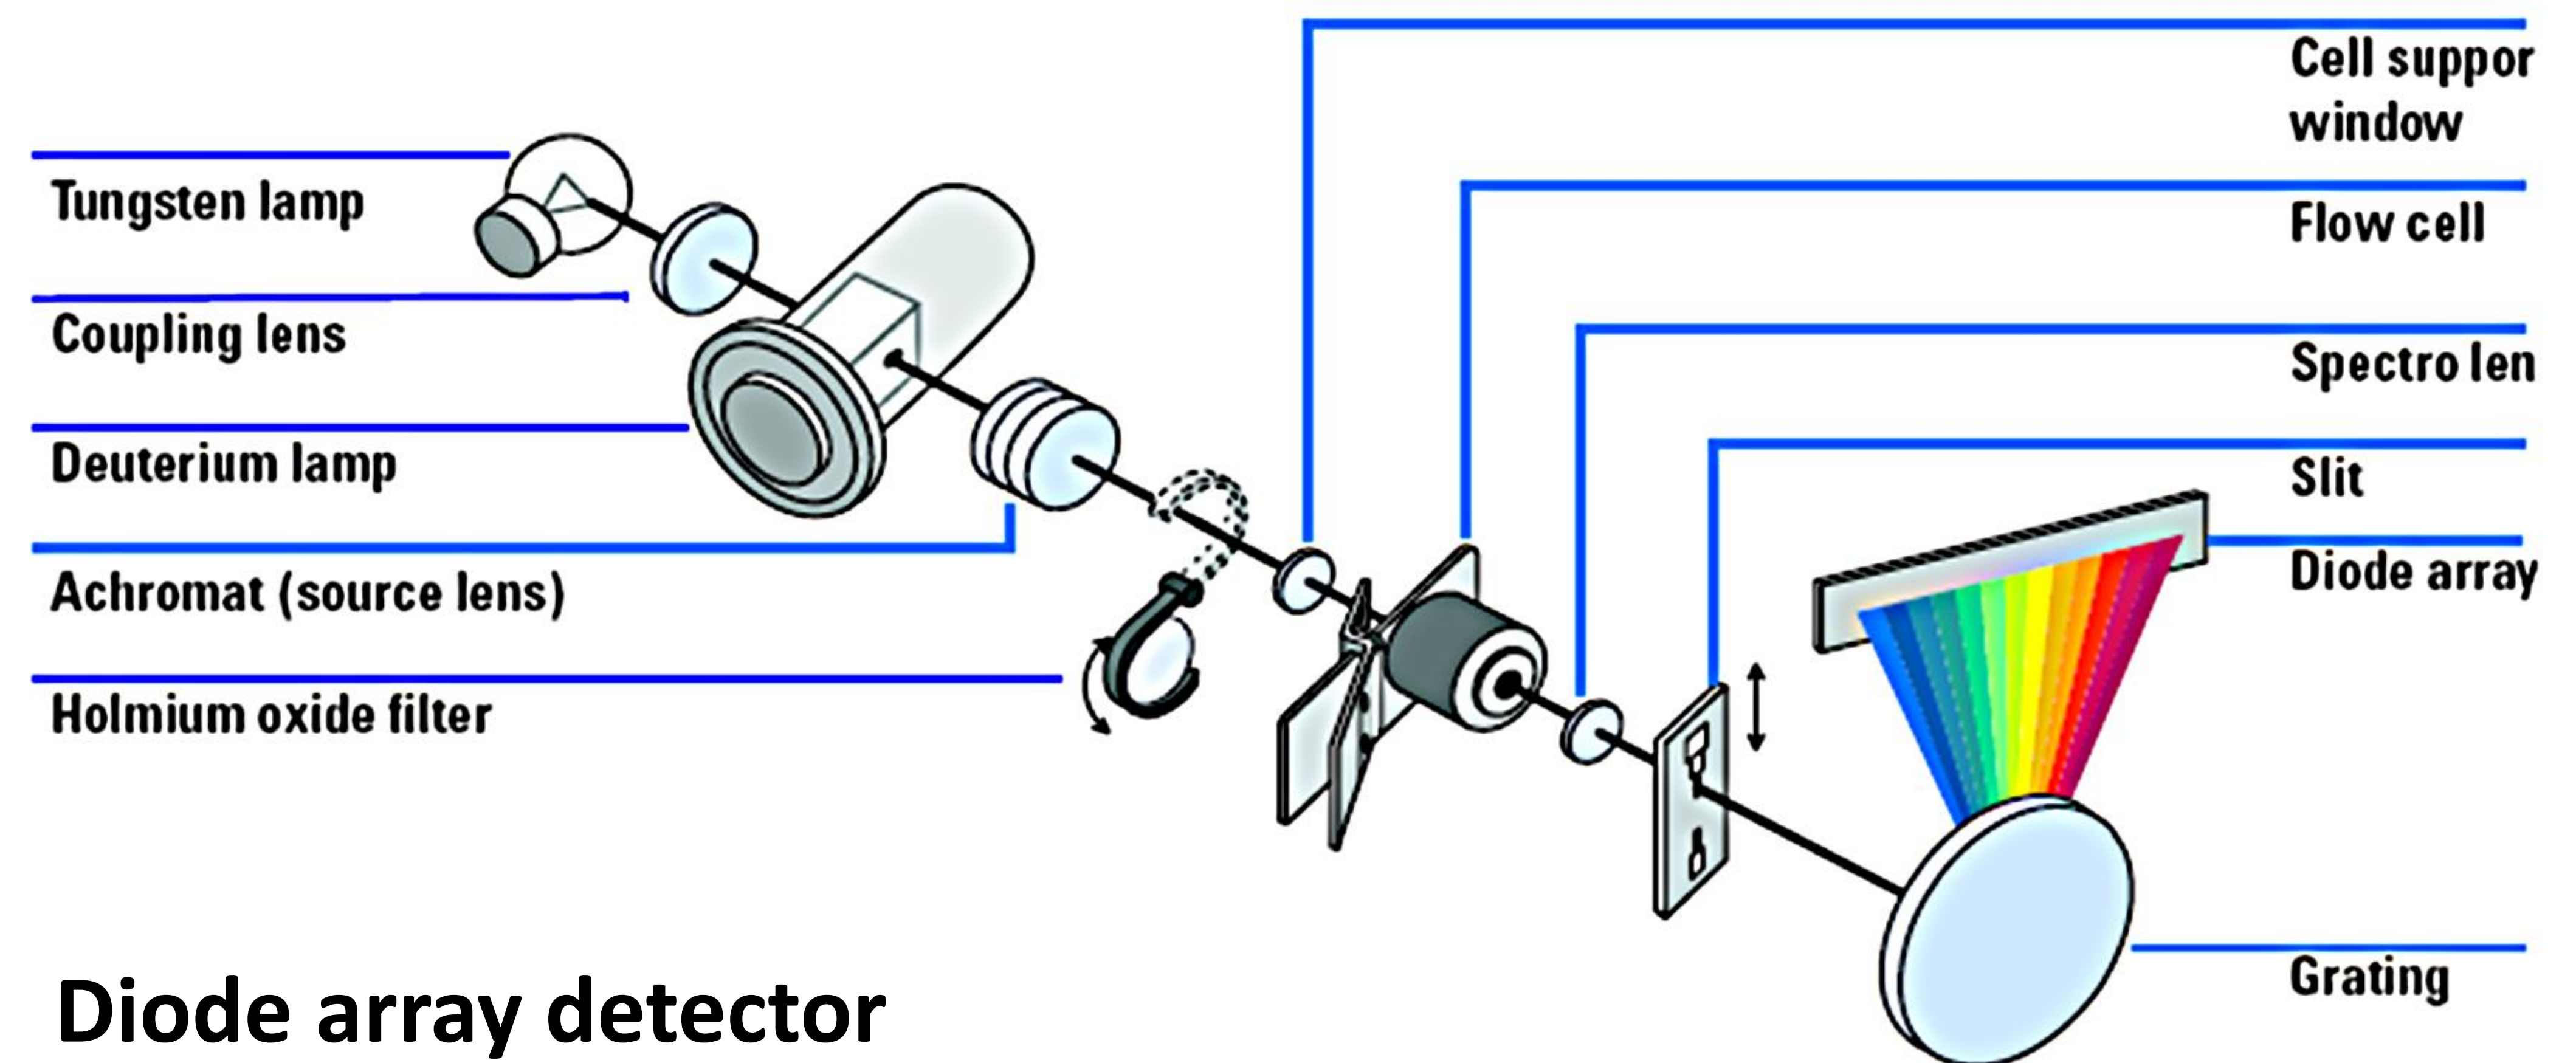

Diode array detector optical system